



NACIONALNI FORENZIČNI LABORATORIJ
NATIONAL FORENSIC LABORATORY

Vodovodna 95
1000 Ljubljana
SLOVENIJA

T: +386 (0)1 428 44 93
E: nfl@policija.si
www.policija.si


ANALYTICAL REPORT

ALD-52 (C22H27N3O2)

11-acetyl-N,N-diethyl-6-methyl-6,11-diazatetracyclo[7.6.1.0^{2,7}.0^{12,16}]hexadeca-1(16),2,9,12,14-pentaene-4-carboxamide

Remark – other NPS detected: **none**

Sample ID:	1404-16
Sample description:	blotter
Sample type:	collected /RESPONSE -purchasing
Date of sample receipt (M/D/Y):	9/7/2016
Date of entry (M/D/Y) into NFL database:	10/26/2017
Report ¹ updates (if any) will be published here:	http://www.policija.si/apps/nfl_response_web/seznam.php

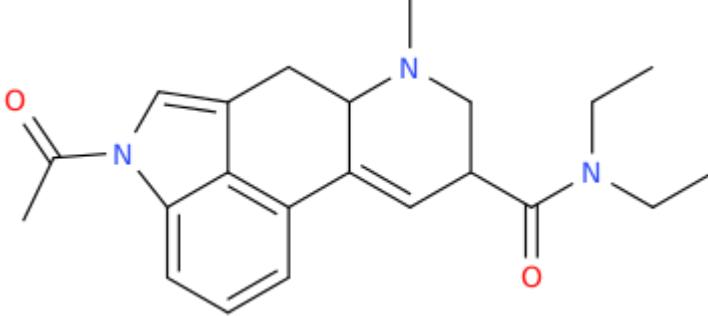Substance identified - structure ² (base form)	
Systematic name	11-acetyl-N,N-diethyl-6-methyl-6,11-diazatetracyclo[7.6.1.0 ^{2,7} .0 ^{12,16}]hexadeca-1(16),2,9,12,14-pentaene-4-carboxamide
Other names	1-acetyllysergic acid diethylamide, 4-acetyl-N,N-diethyl-7-methyl-6,6a,8,9-tetrahydroindolo[4,3-fg]quinoline-9-carboxamide
Formula (per base form)	C22H27N3O2
M _w (g/mol)	365,48
Salt form/anions detected	na
StdInChIKey (per base form)	FJOWXGYLIWJFCH-UHFFFAOYSA-N
Other NPS detected	none
Additional info (purity..)	

¹ This report has been produced with the financial support of the Prevention of and fight against crime Programme of the European Union (grant agreement number JUST/2013/ISEC/DRUGS/AG/6413). The contents of this report are the sole responsibility of the National Forensic Laboratory and can in no way be taken to reflect the views of the European Commission.

² Created by OPSIN free tool: <http://opsin.ch.cam.ac.uk/> DOI: 10.1021/ci100384d

Report updates

date	comments (explanation)

Instrumental methods (if applied) in NFL

1. GC-MS (Agilent): GC-method is RT locked to tetracosane (9.258 min). Injection volume 1 ml and split mode (1:50). Injector temperature: 280 °C. Chromatographic separation: on column HP1-MS (100% dimethylpolysiloxane), length 30 m, internal diameter 0.25 mm, film thickness 0.25 µm. Carrier gas He: flow-rate 1.2 ml/min. GC oven program: 170 °C for 1 min, followed by heating up to 190 °C at rate 8 °C/min, then heating up to 293 °C at a rate of 18 °C/min, hold for 7.1 min, then heating at 50 °C/min up to 325 °C and finally 6.1 min isothermal. MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300 until 6 min) amu.

2. HPLC-TOF (Agilent): 6230B TOF with Agilent 1260 Infinity HPLC with binary pump, column: Zorbax Eclipse XDB-C18, 50 x 4.6 mm, 1.8 micron. Mobile phases (A) 0.1% formic acid and 1mM ammonium formate in water; (B) 0.1% formic acid in methanol (B). Gradient: starting at 5% B, changing to 40% B over 4 min, then to 70% over 2 min and in 5 min to 100%, hold 1 min and back to 5%, equilibration for 1.7 min. The flow rate: 1.0 ml/min; Injection volume 1 µl. MS parameters: 2GHz, Extended Dynamic range mode to a maximum of 1700 amu, acquisition rate 1.30 spectra/sec. Sample ionisation: by Agilent Jet Stream technology (Dual AJS ESI). Ion source: positive ion scan mode with mass scanning from 82 to 1000 amu. Other TOF parameters: drying gas (N2) and sheath temperature 325 °C; drying gas flow rate 6 l/min; sheath gas flow rate 8 l/min; nebulizer 25 psig; Vcap. 4000 V; nozzle 2000 V; skimmer 65 V; fragmentor 175 V and Octopole RF 750 V.

3. FTIR-ATR (Perkin Elmer): scan range 4000-400 cm⁻¹; resolution 4cm⁻¹

4. GC- (MS)-IR condensed phase (GC-MS (Agilent) & IR (Spectra analyses-Danny))

GC-method: Injection volume 1 ml and split mode (1:5). Injector temperature 280 °C. Chromatographic separation as above (1). Split MS : IR = 1: 9.

MSD source EI = 70 eV. GC-MS transfer line T= 235 °C, source and quadropole temperatures 280 °C and 180 °C, respectively. Scan range m/z scan range: from 50 (30 until 6 min.) to 550 (300) amu.

IR (condensed (solid) phase): IR scan range 4000 to 650, resolution 4 cm⁻¹.

5. IC (anions) (Thermo Scientific, Dionex ICS 2100), Column: IonPac AS19, 2 x 250mm; Eluent: 10mM from 0 to 10 min, 10-58 mM from 10 to 40min; Flow rate: 0.25 ml/min; Temperature: 30°C; Suppressor: AERS 500 2mm, suppressor current 13mA; Inj. Volume: 25 µl


Supporting information

Solubility in	result/remark
CH ₂ Cl ₂	
MeOH	
H ₂ O	

Analytical technique:	applied	remarks
GC-MS (EI ionization)	+	NFL GC-RT (min): 16,95 BP(1): 263; BP(2): 72,BP(3) :221,
HPLC-TOF	+	Exact mass (theoretical): 365,2104; measured value Δppm:-0,02; formula:C22H27N3O2
FTIR-ATR	-	direct measurement (sample as received)
FTIR (condensed phase) always as base form	+	
IC (anions)	-	
NMR (in FKKT)	-	
validation		
other		

ANALYTICAL RESULTS

MS (EI) – background substracted

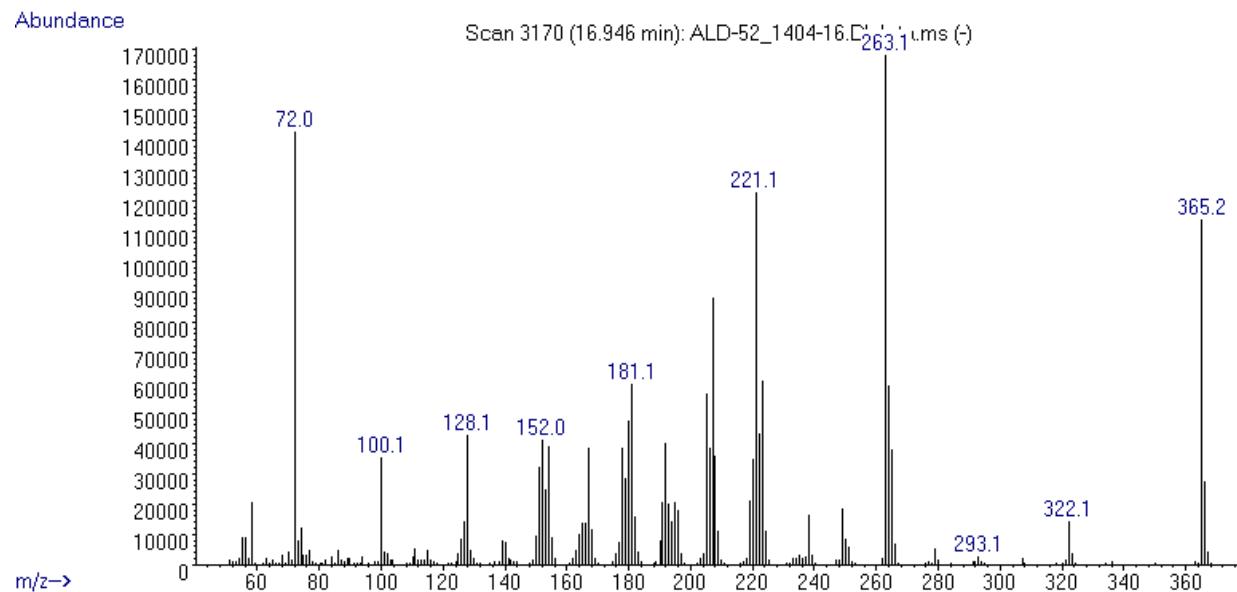

IR (condensed phase – after chromatographic separation)

